

FIGURE 1

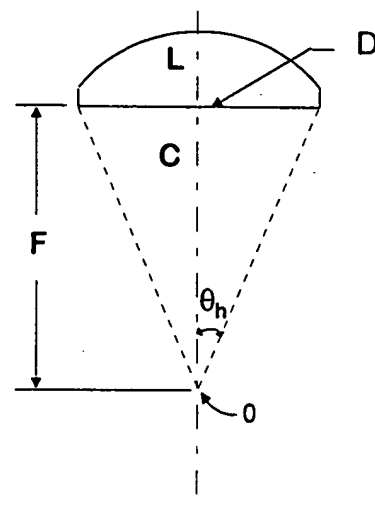


FIGURE 2

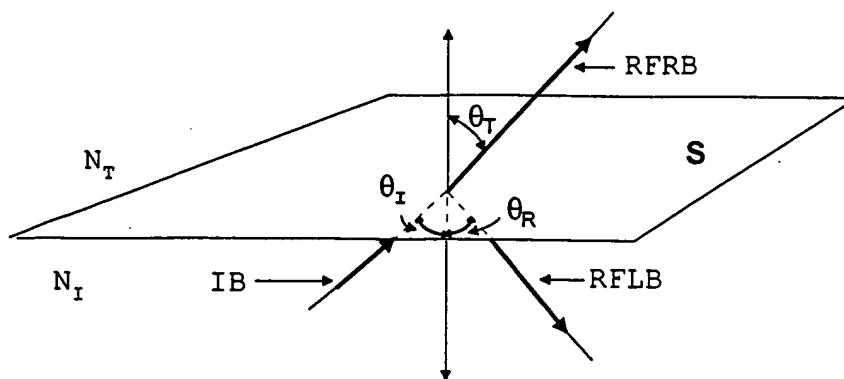


FIGURE 3

FOSTED 627 FEB 60

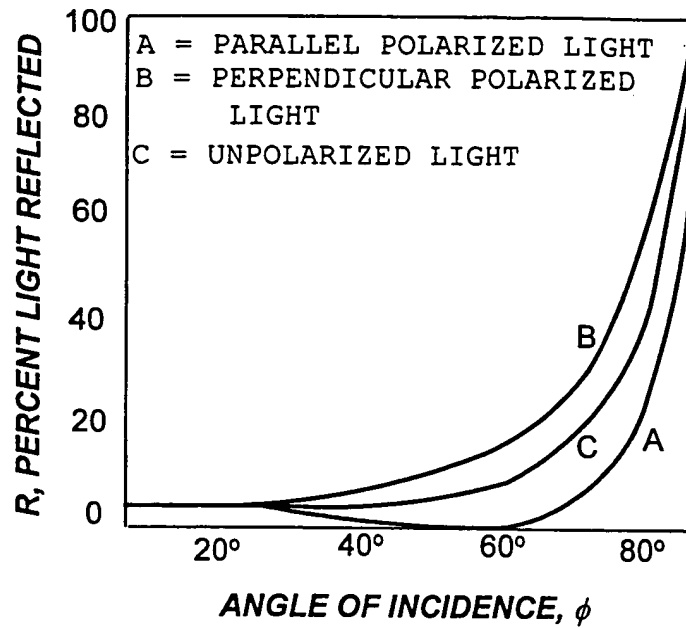


FIGURE 4A

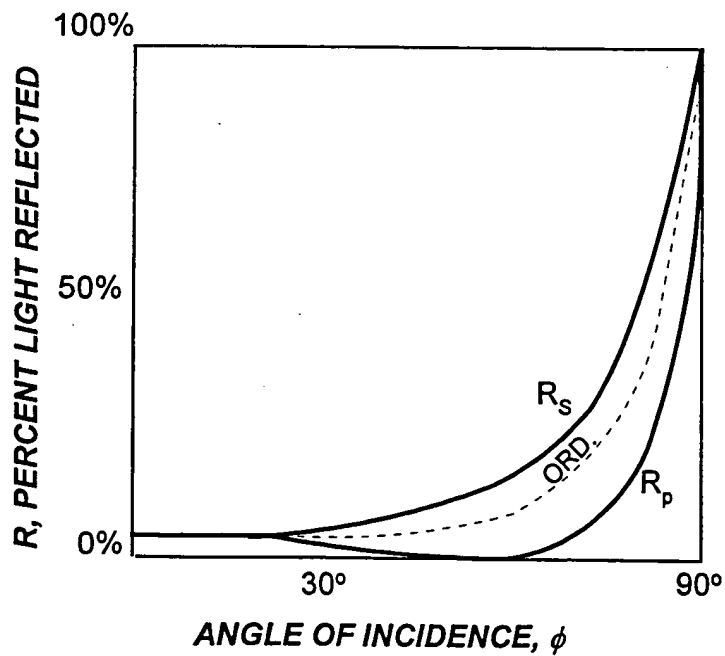


FIGURE 4B

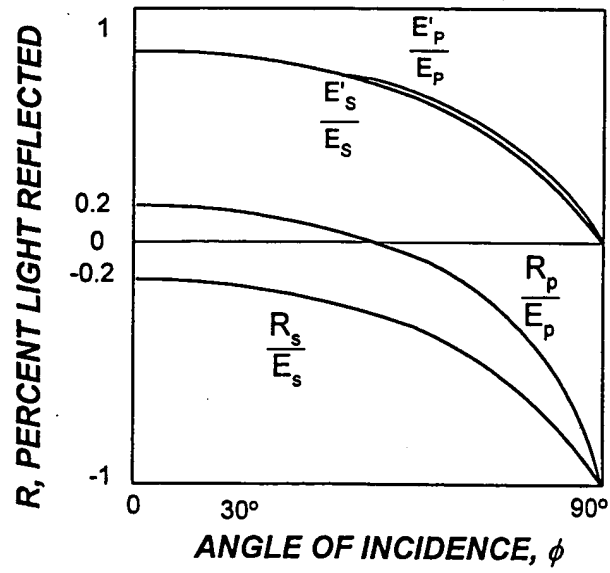


FIGURE 4C

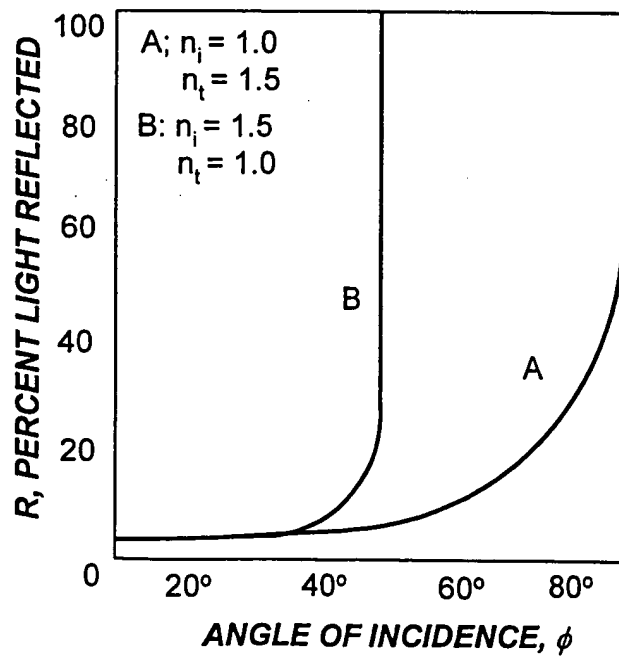


FIGURE 5A

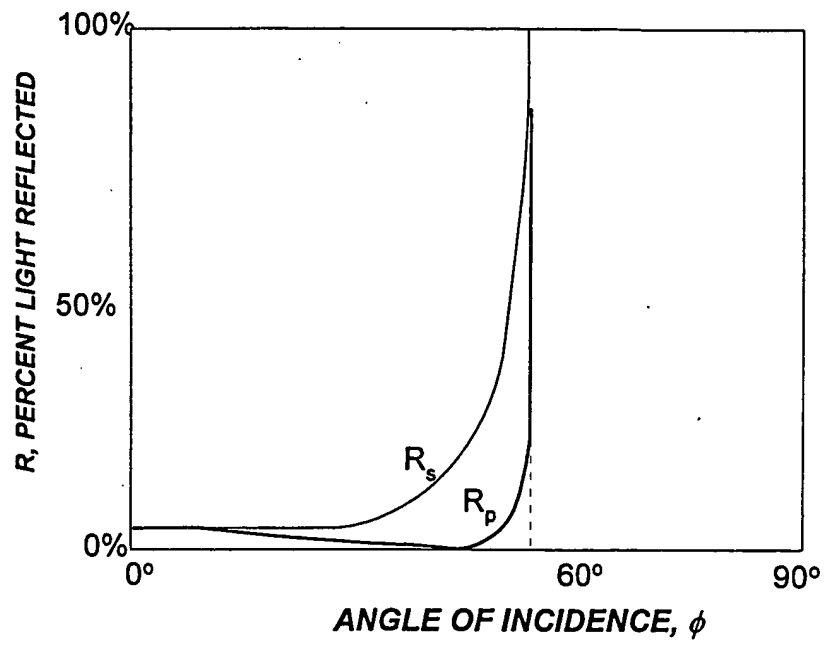


FIGURE 5B

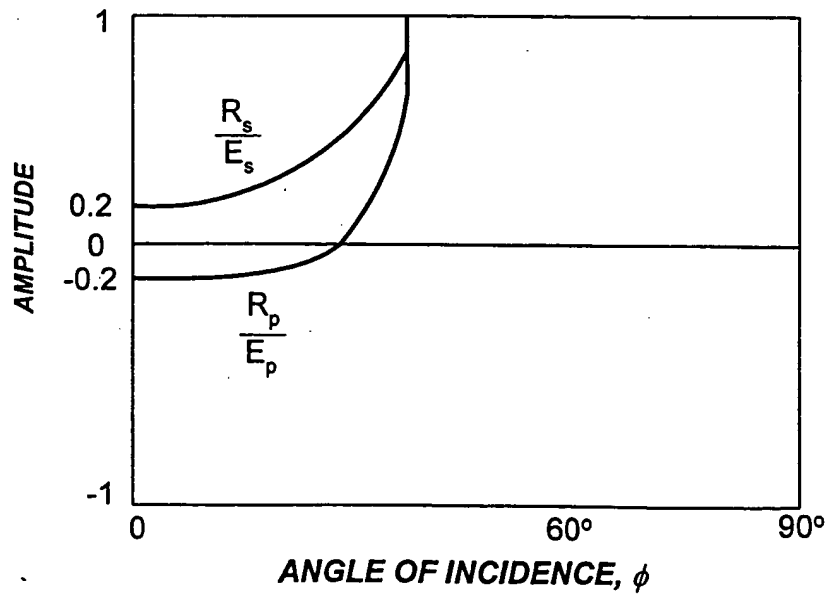


FIGURE 5C

109430-024E660

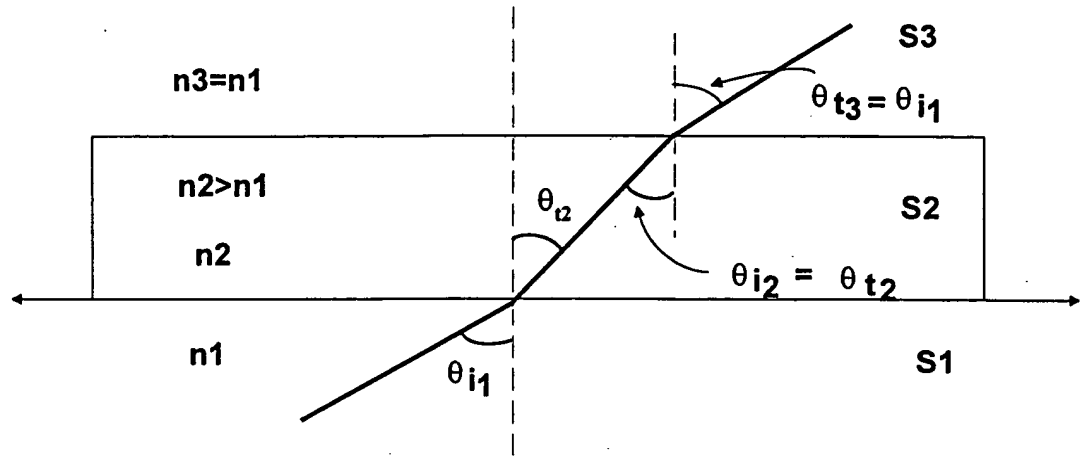


FIGURE 6

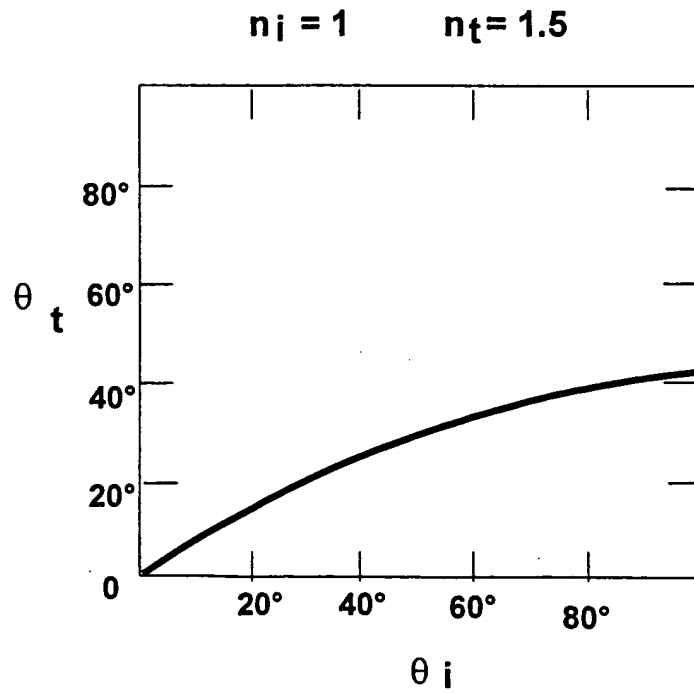


FIGURE 7

00931729-084604

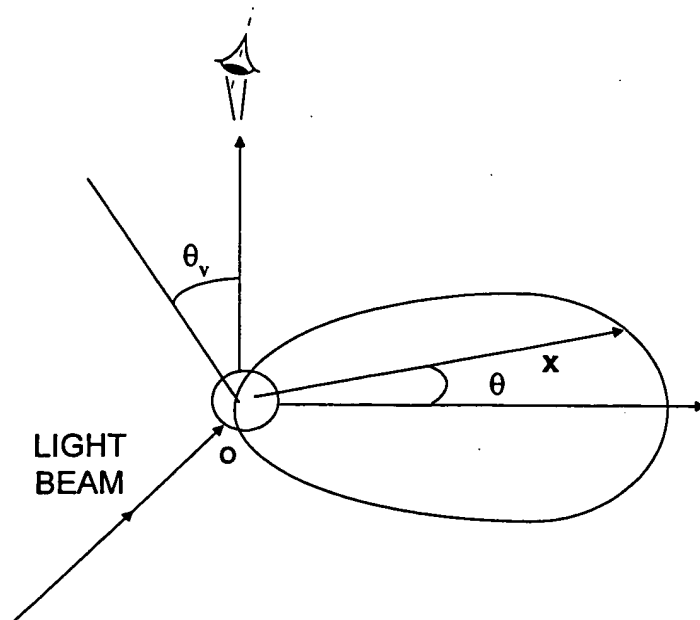


FIGURE 8

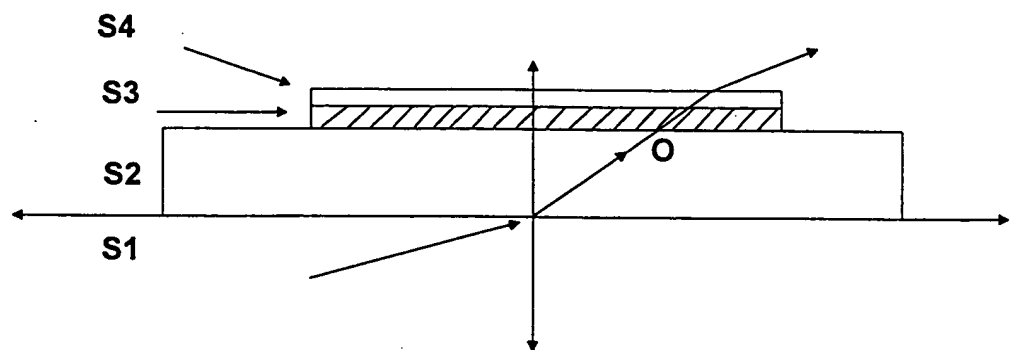


FIGURE 9

TOP SECRET 6247E990

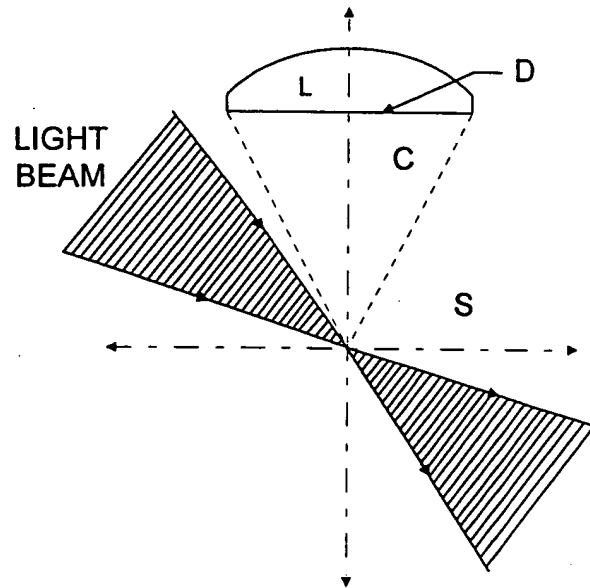


FIGURE 10

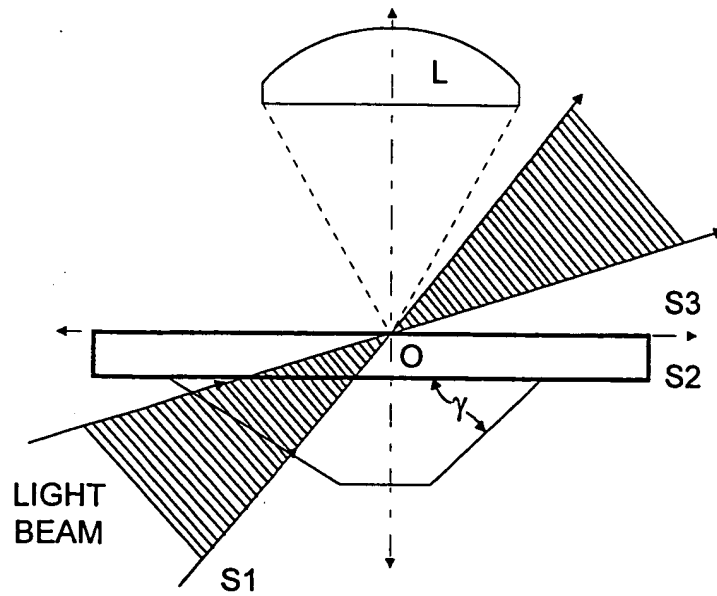


FIGURE 11

FOUO-624260

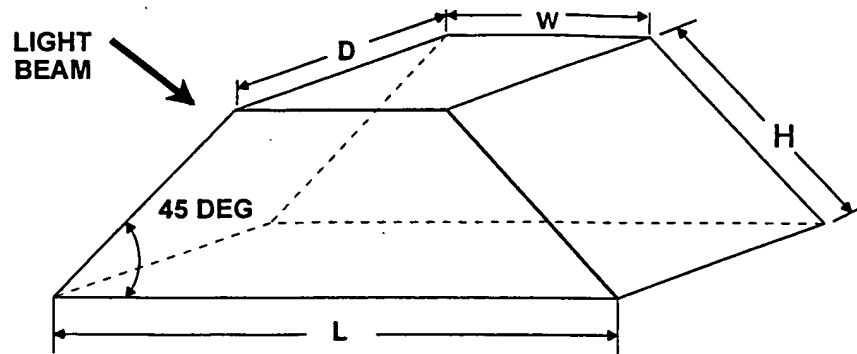


FIGURE 12A

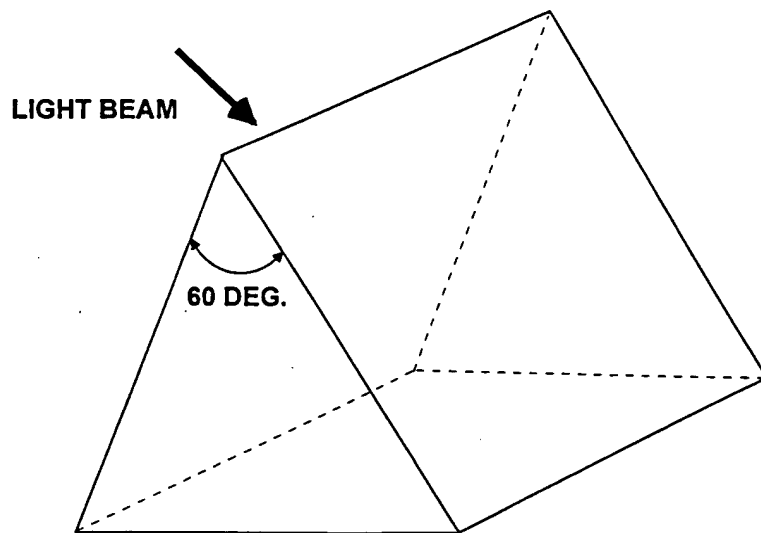


FIGURE 12B

TOP SECRET

9/30

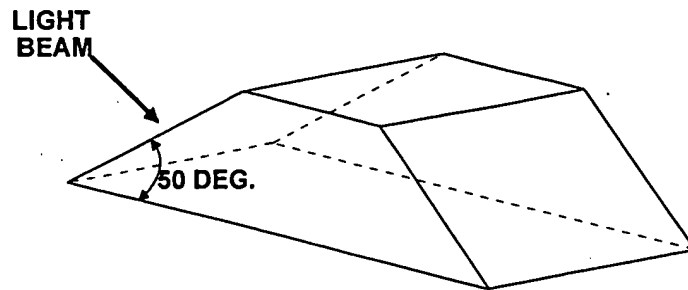


FIGURE 12C


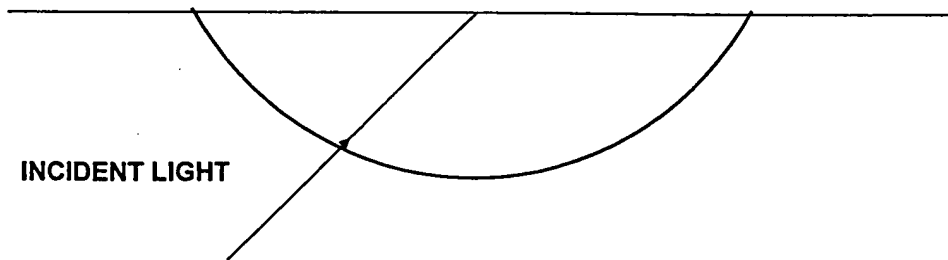


FIGURE 12D

FOSTED-624E60

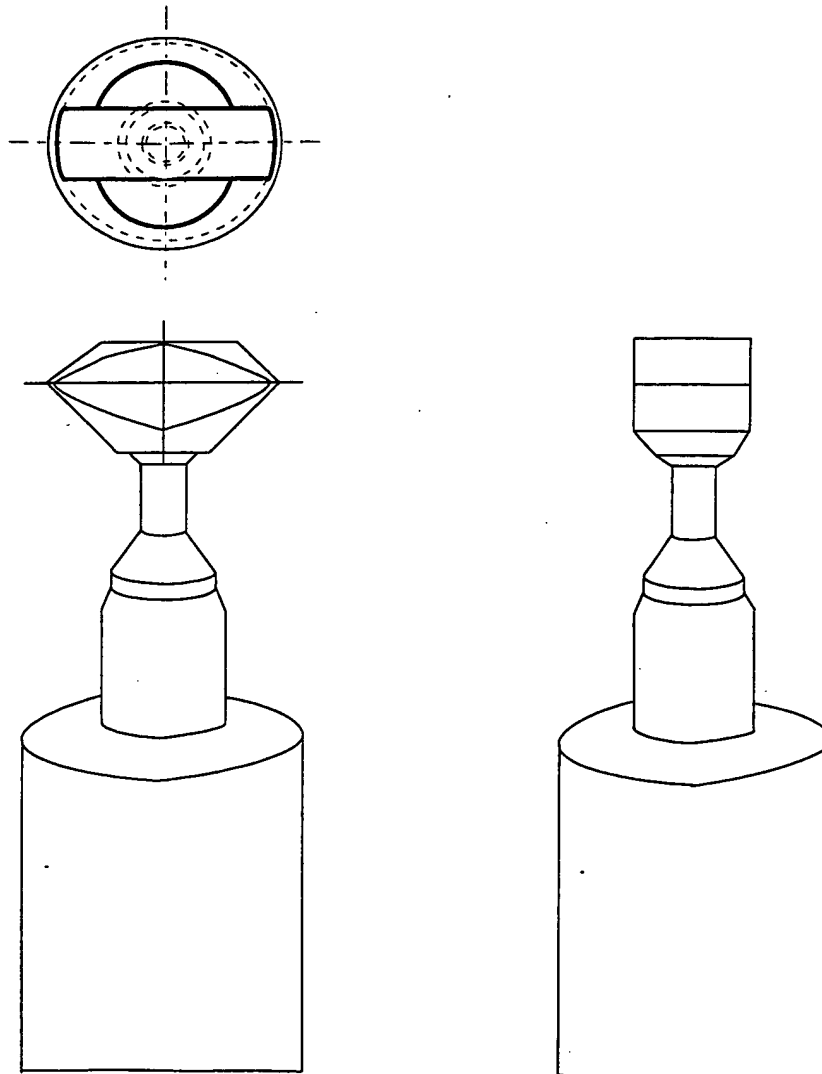

NOT TO SCALE

FIGURE 12E

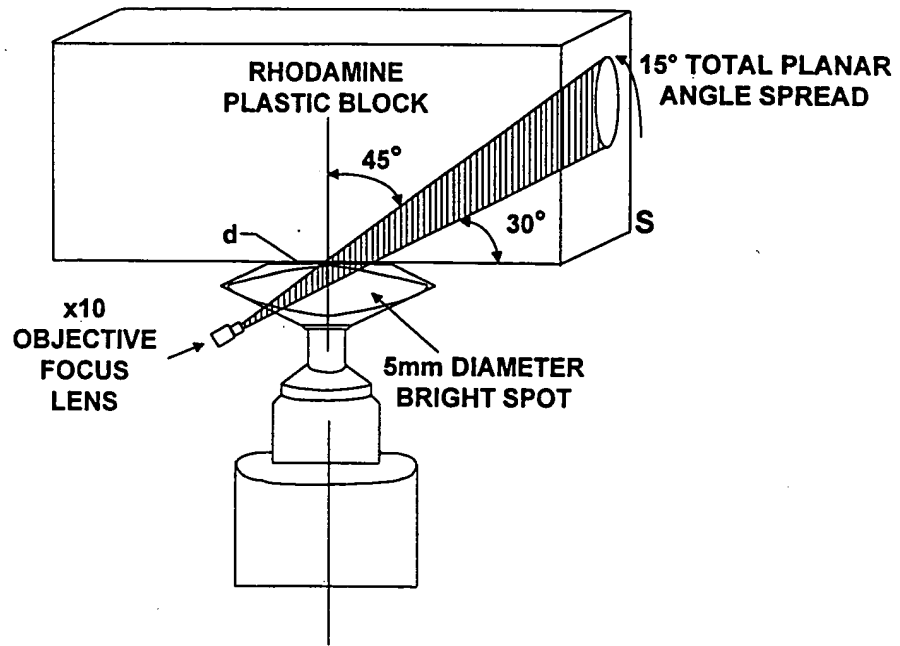


FIGURE 13

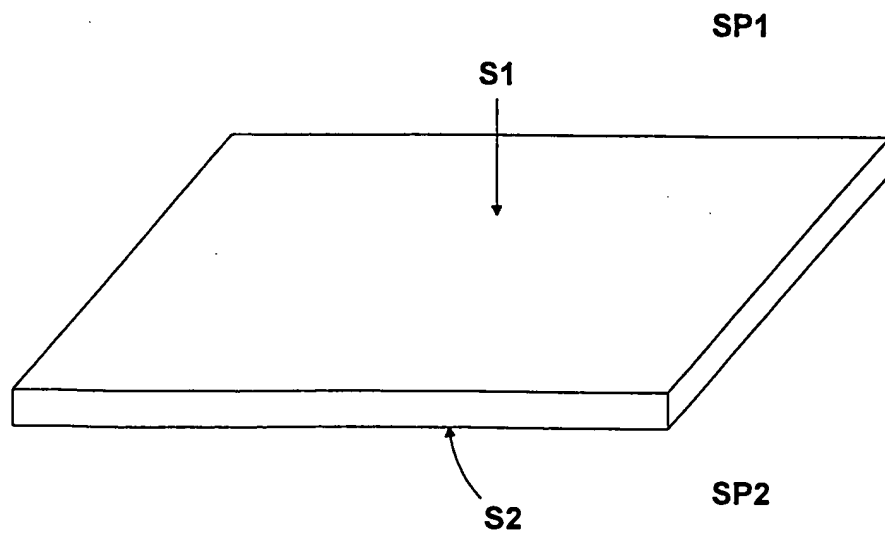


FIGURE 14

1093429-081501

12/30

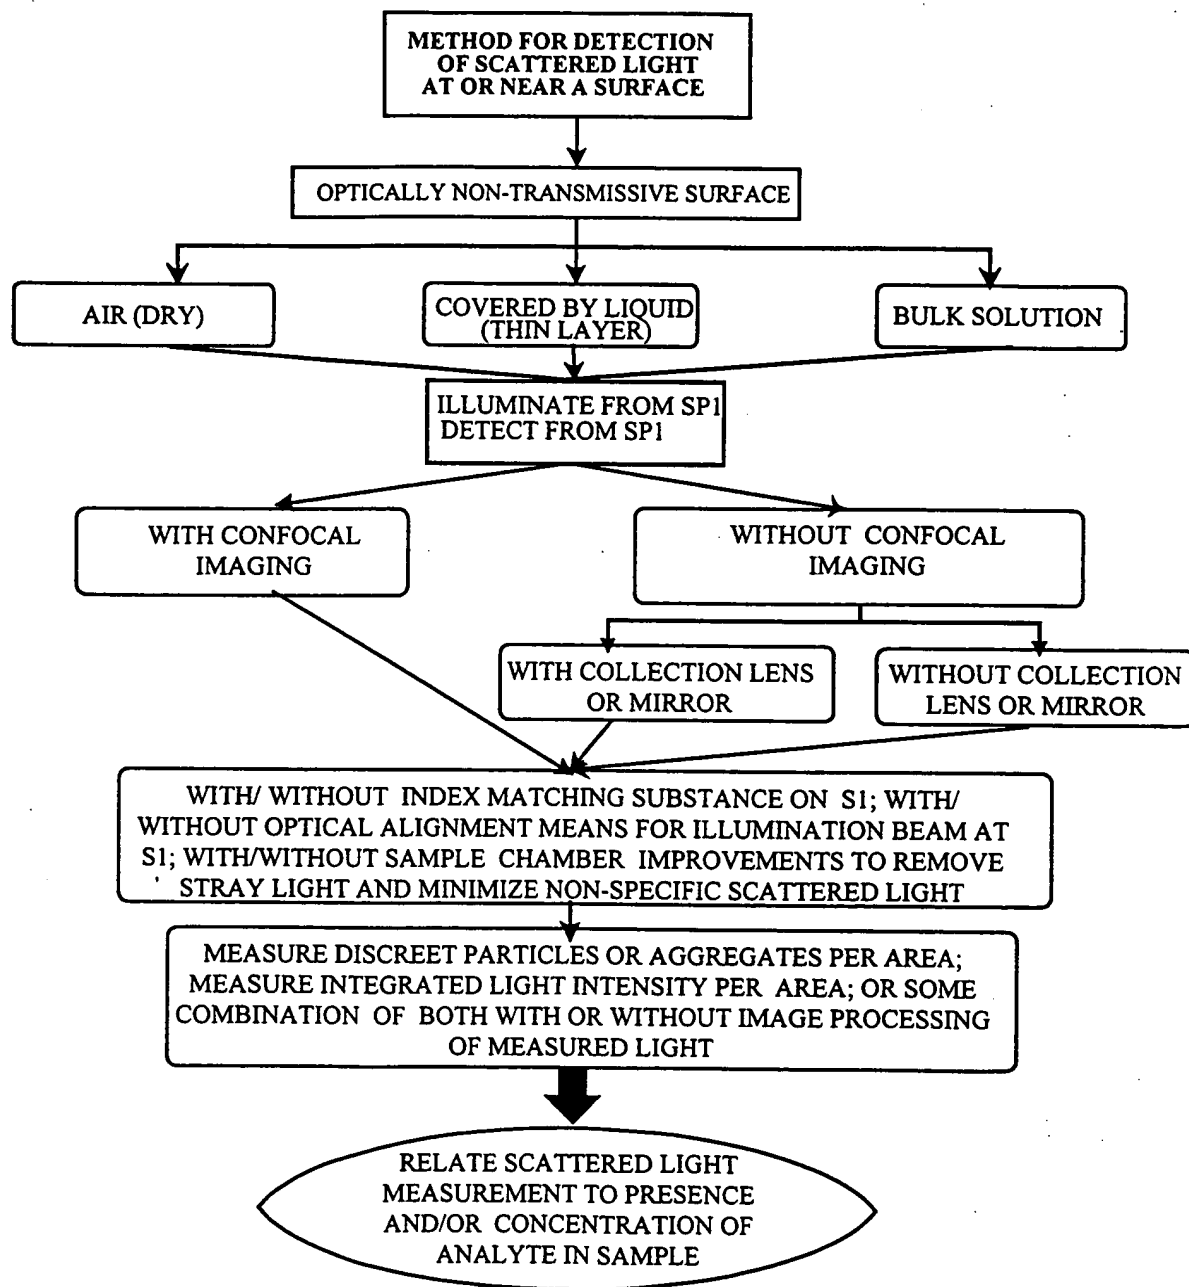


FIGURE 15A

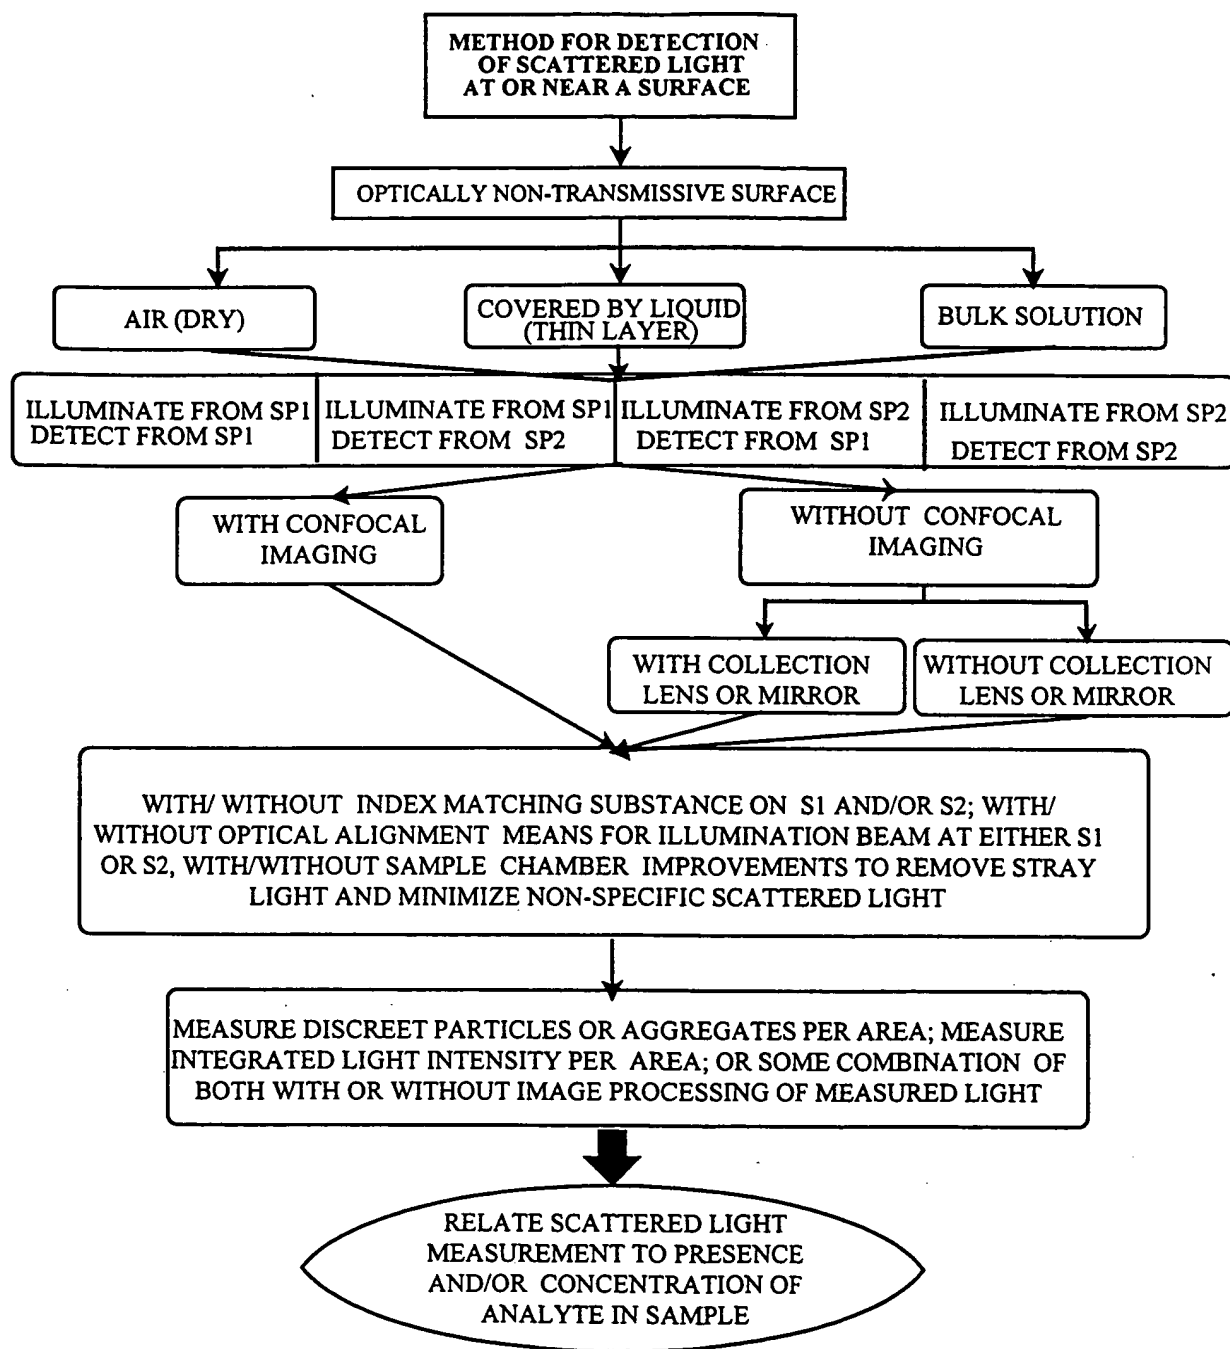


FIGURE 15B

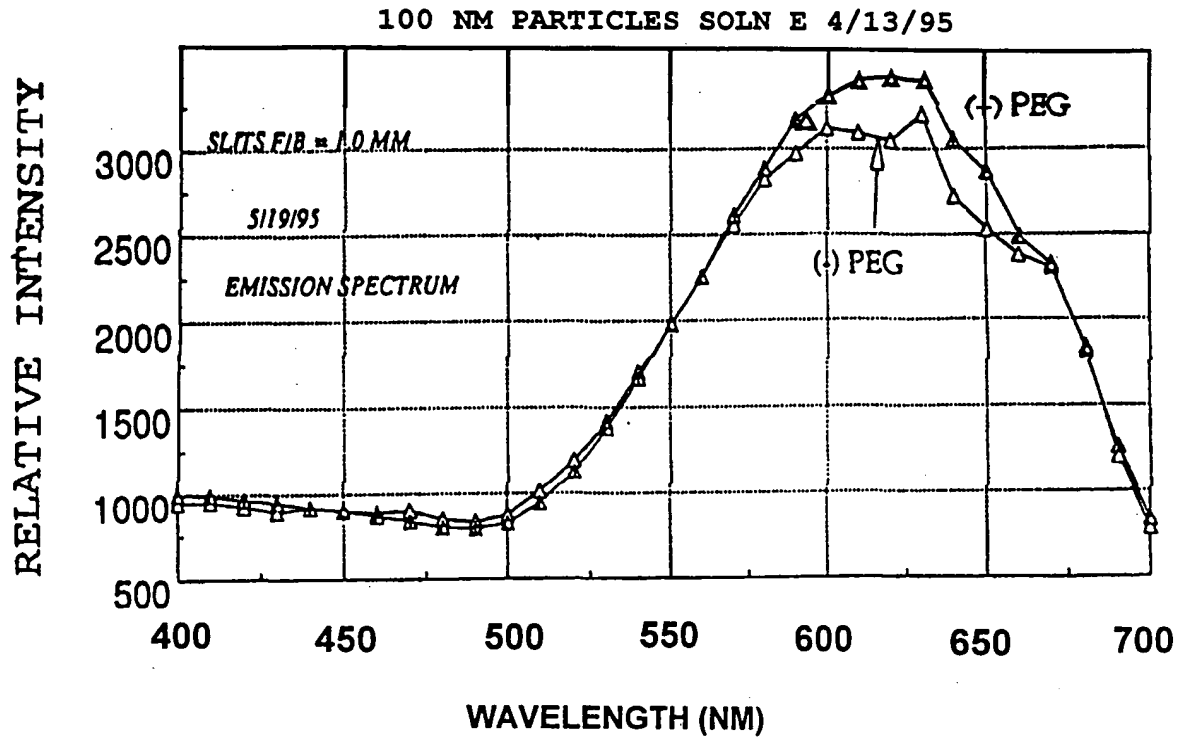


FIGURE 16

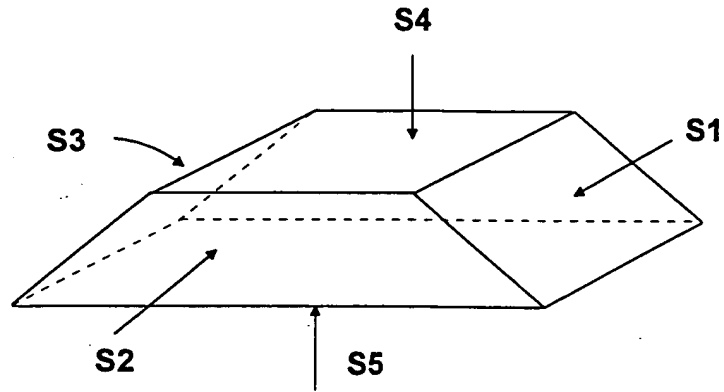


FIGURE 17

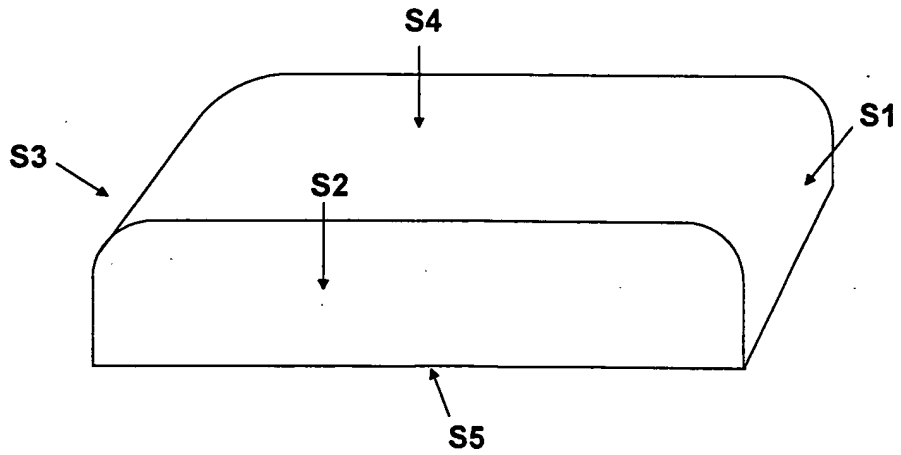


FIGURE 18

FIGURE 18

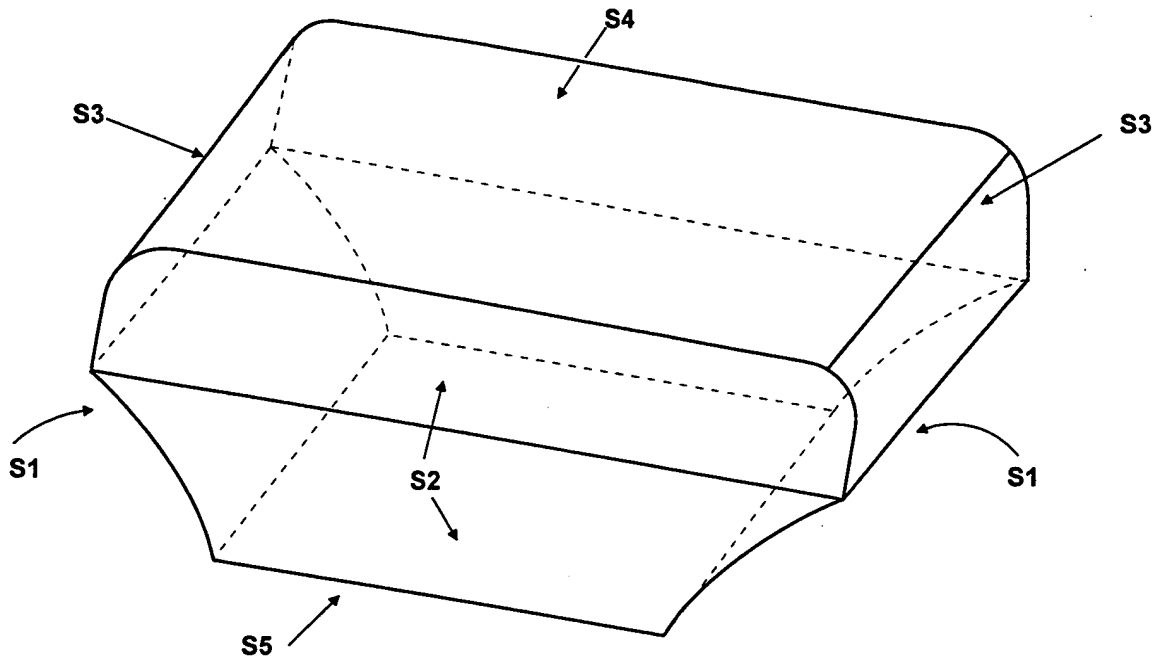


FIGURE 19

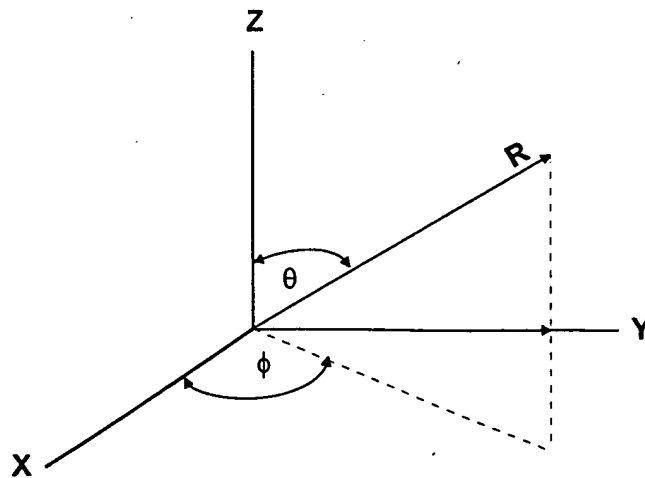


FIGURE 20

00934729-084604

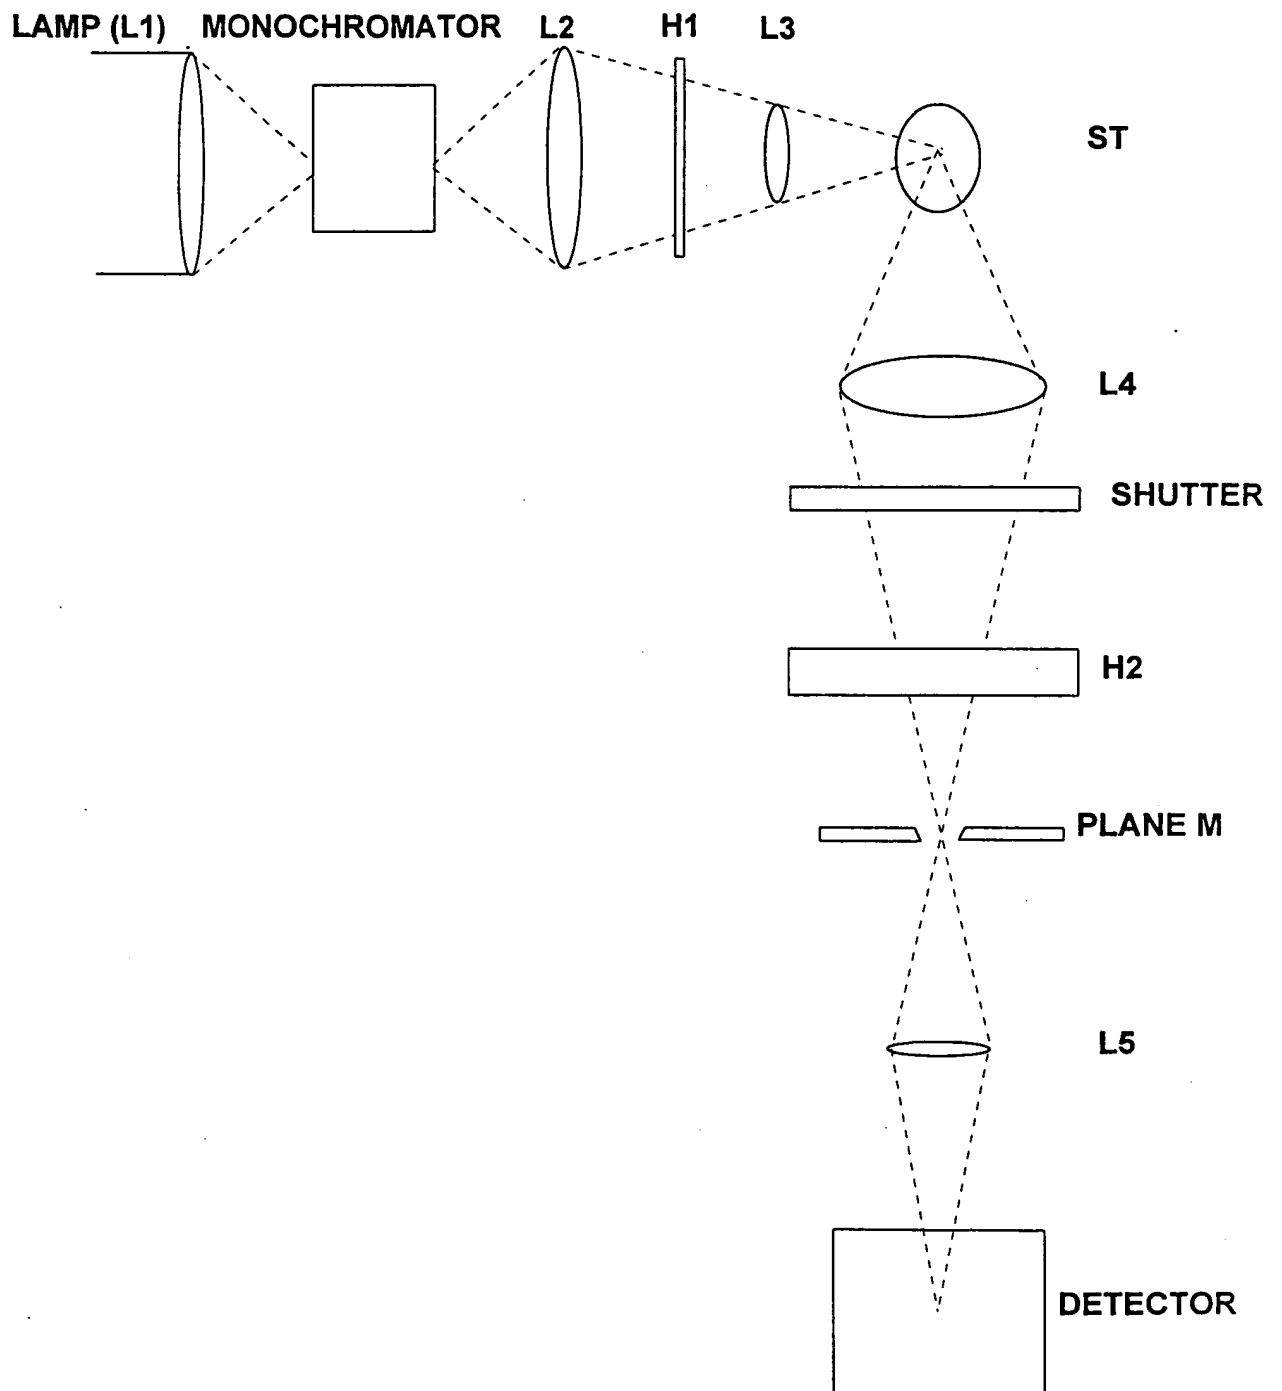


FIGURE 21

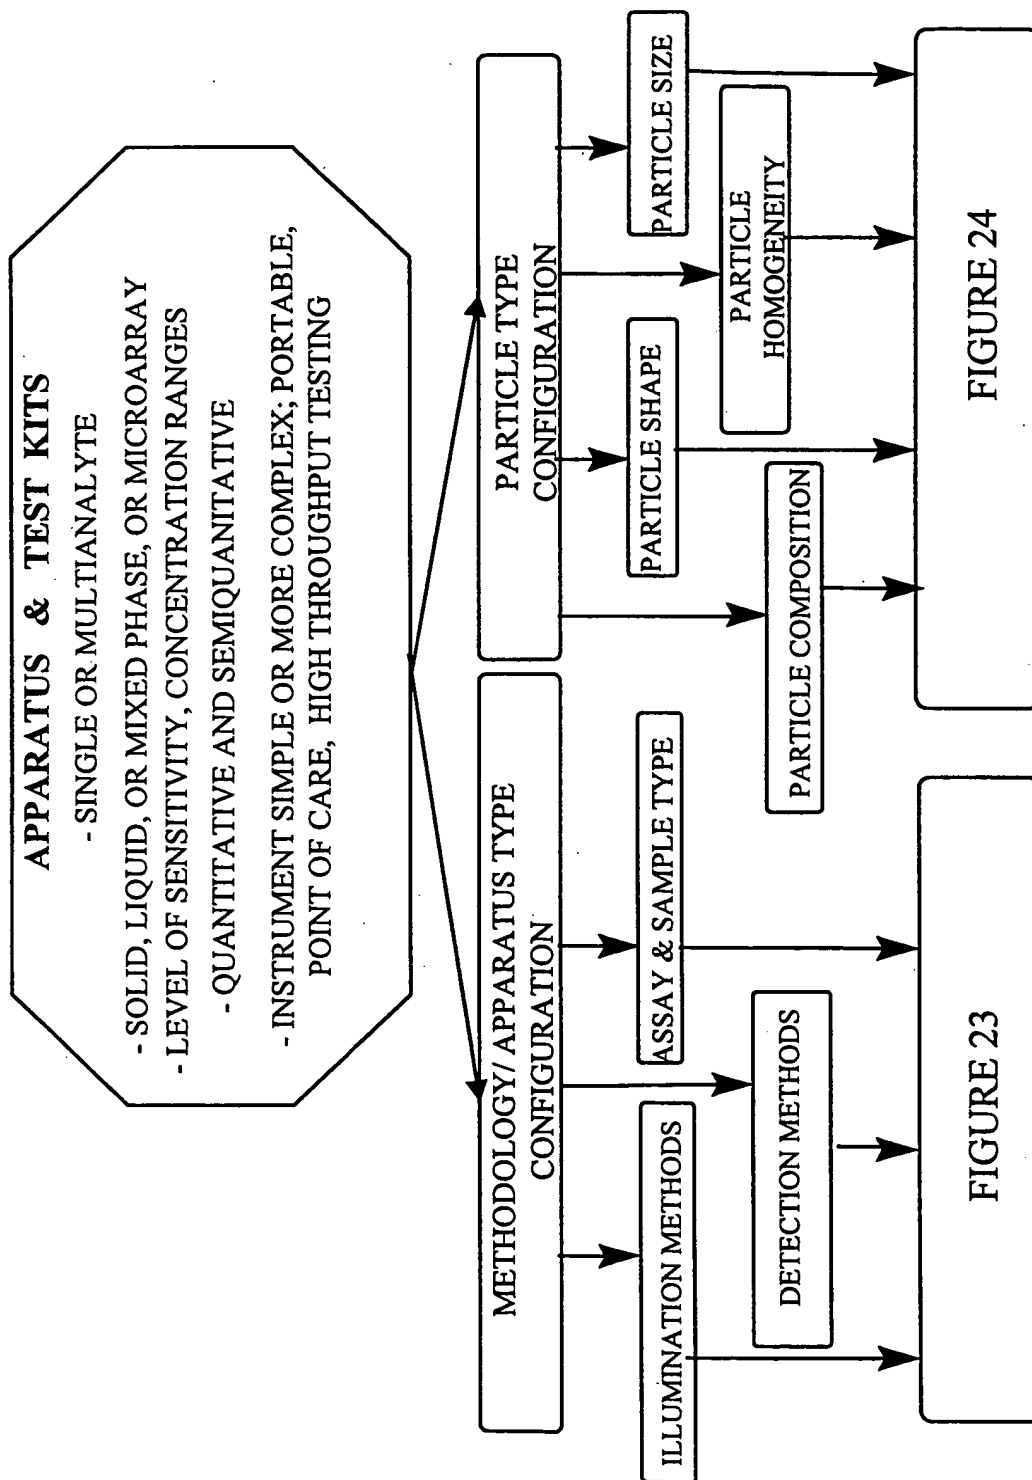


FIGURE 22

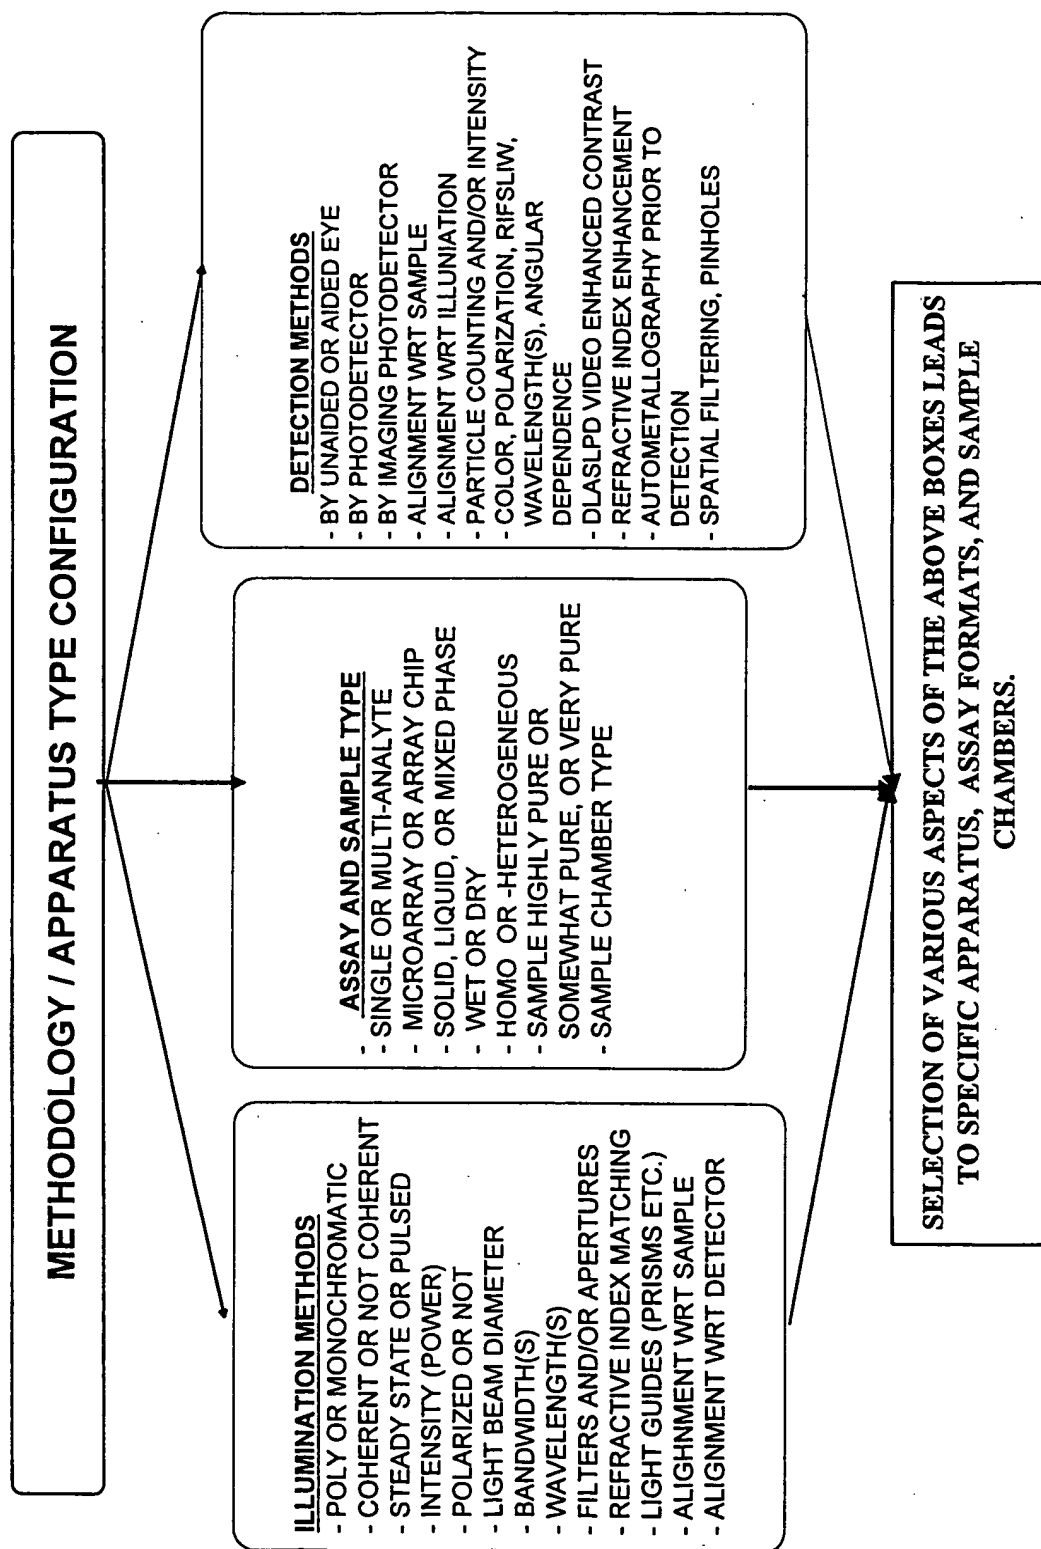


FIGURE 23

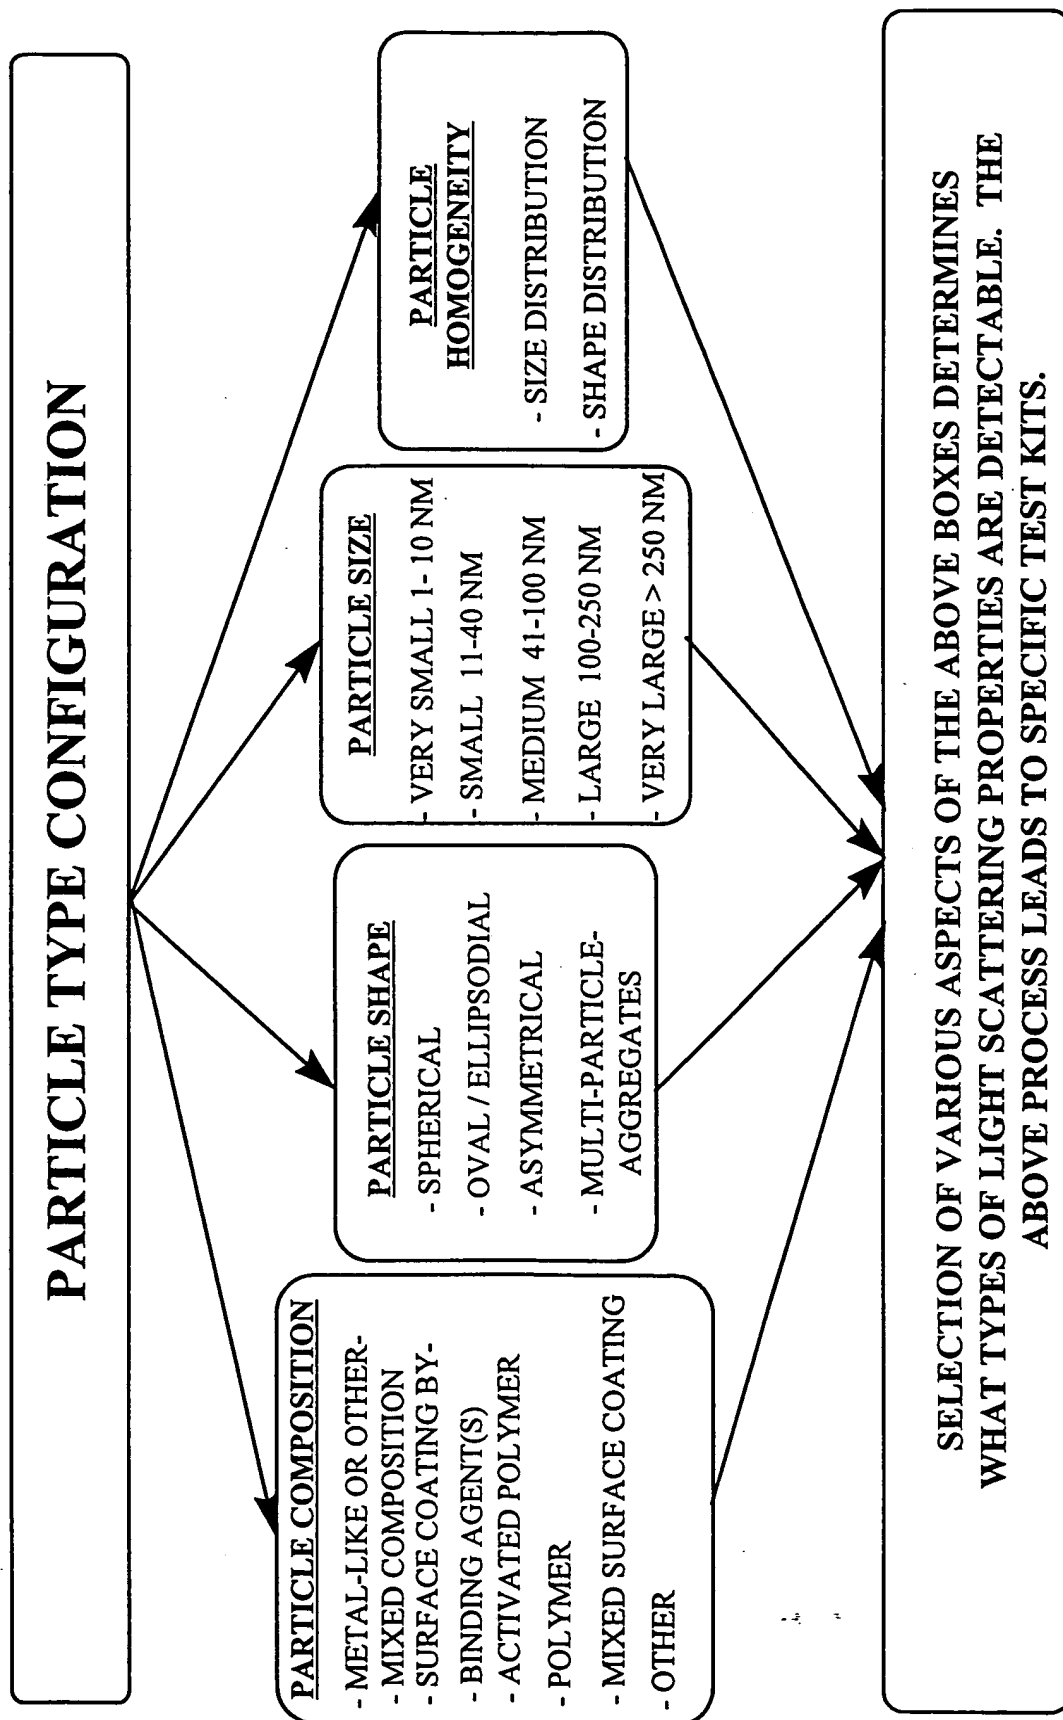


FIGURE 24

**PRACTICE OF INVENTION
TO A SPECIFIC DIAGNOSTIC NEED
LEADING TO SPECIFIC APPARATUS AND
TEST KITS**

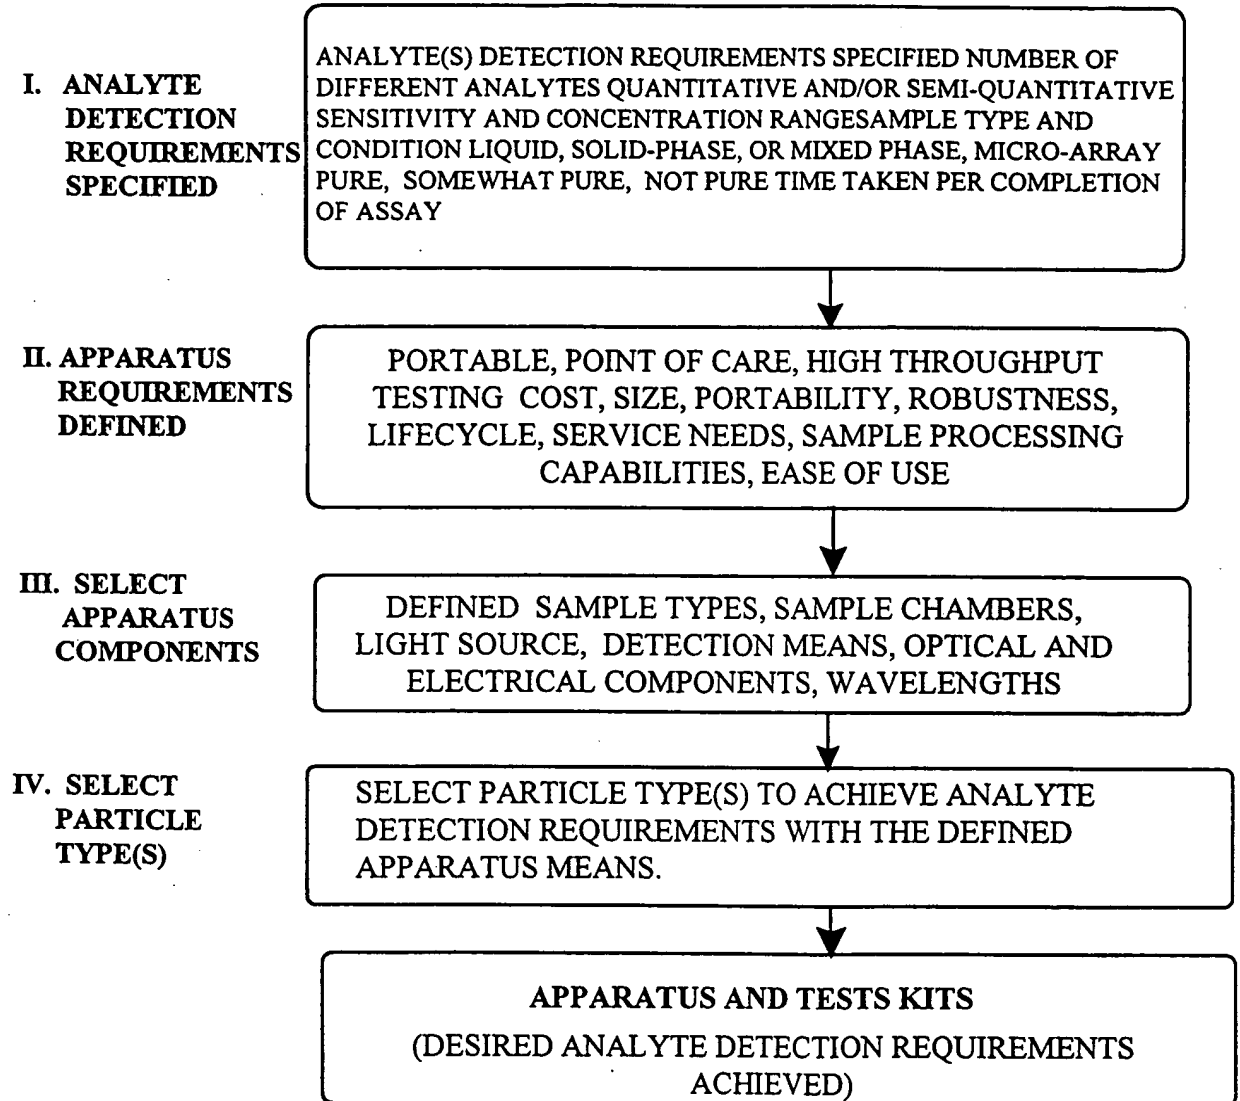
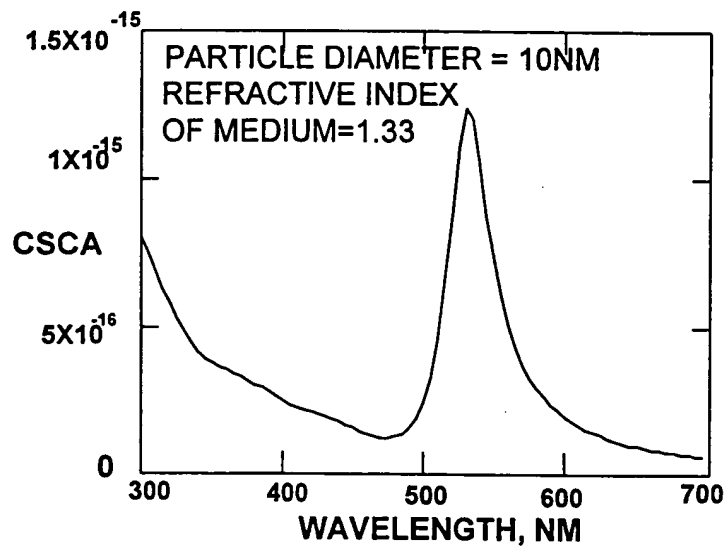
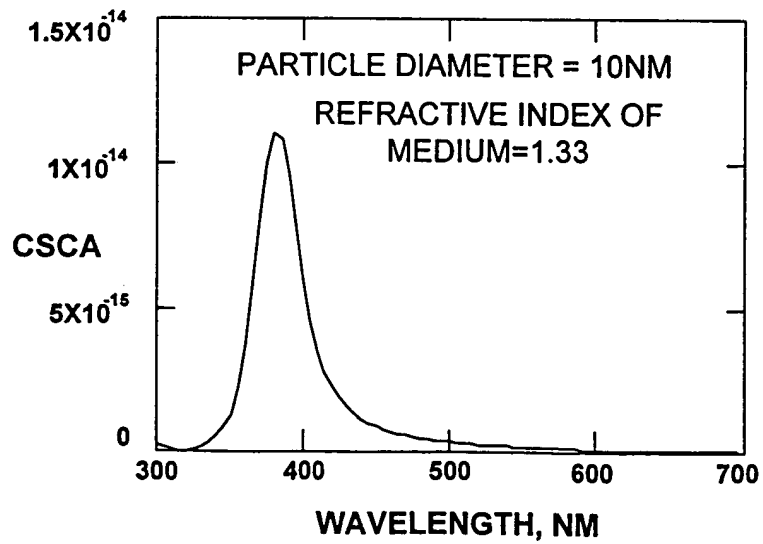
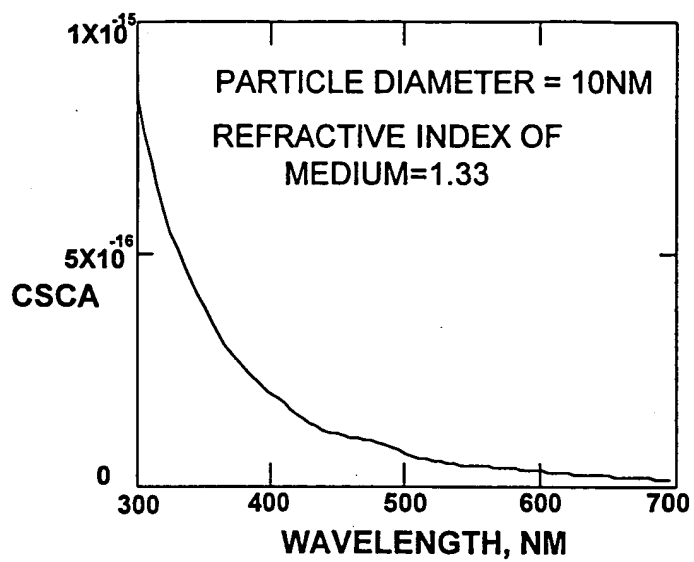
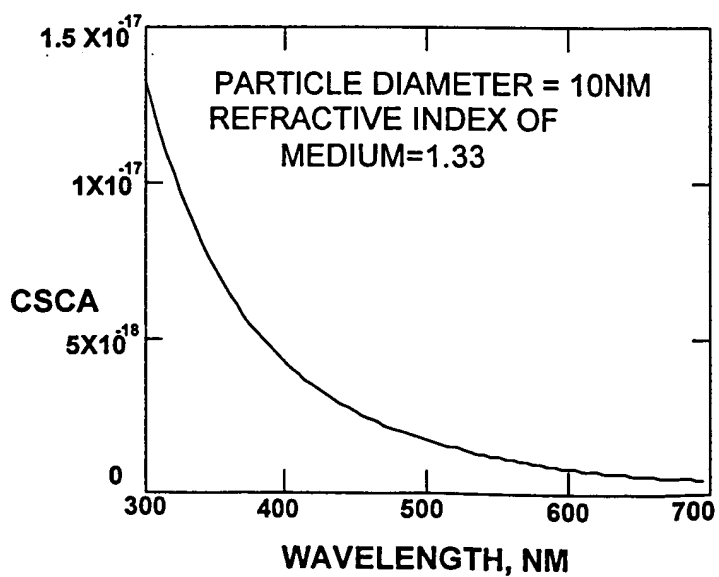


FIGURE 25

GOLD**FIGURE 26A****SILVER****FIGURE 26B**

409490-0242E60

SELENIUM**FIGURE 26C****POLYSTYRENE****FIGURE 26D**

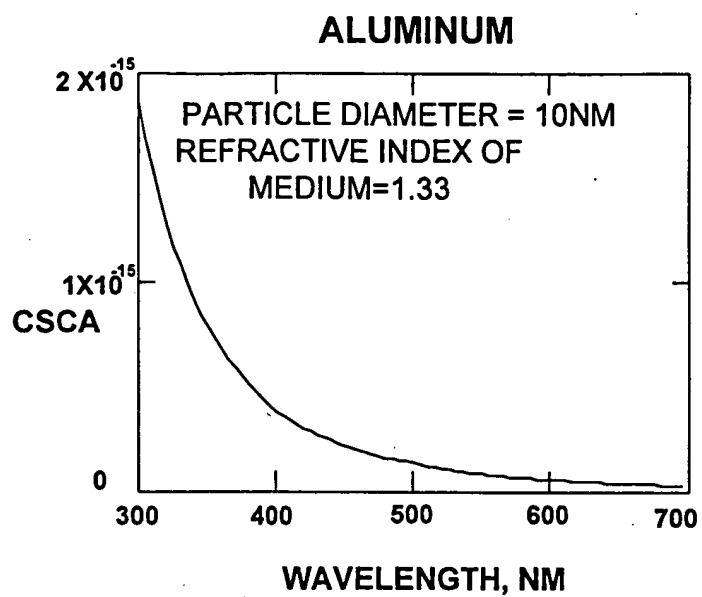


FIGURE 26E

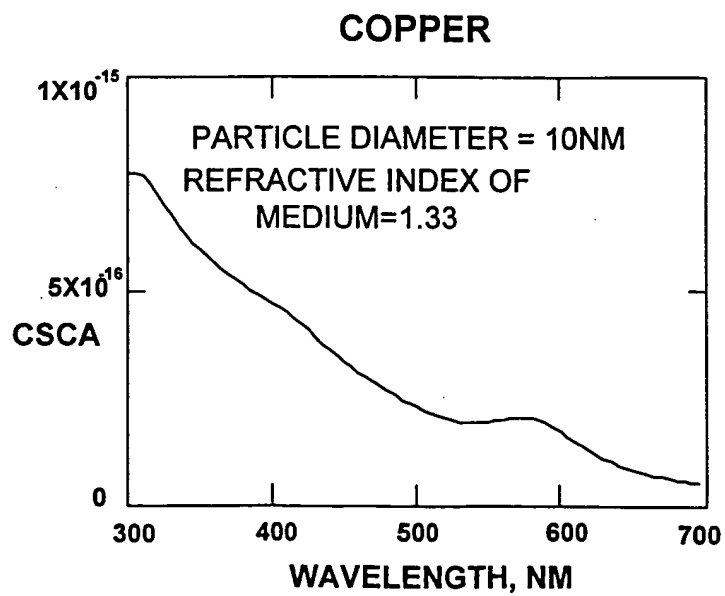


FIGURE 26F

25/30

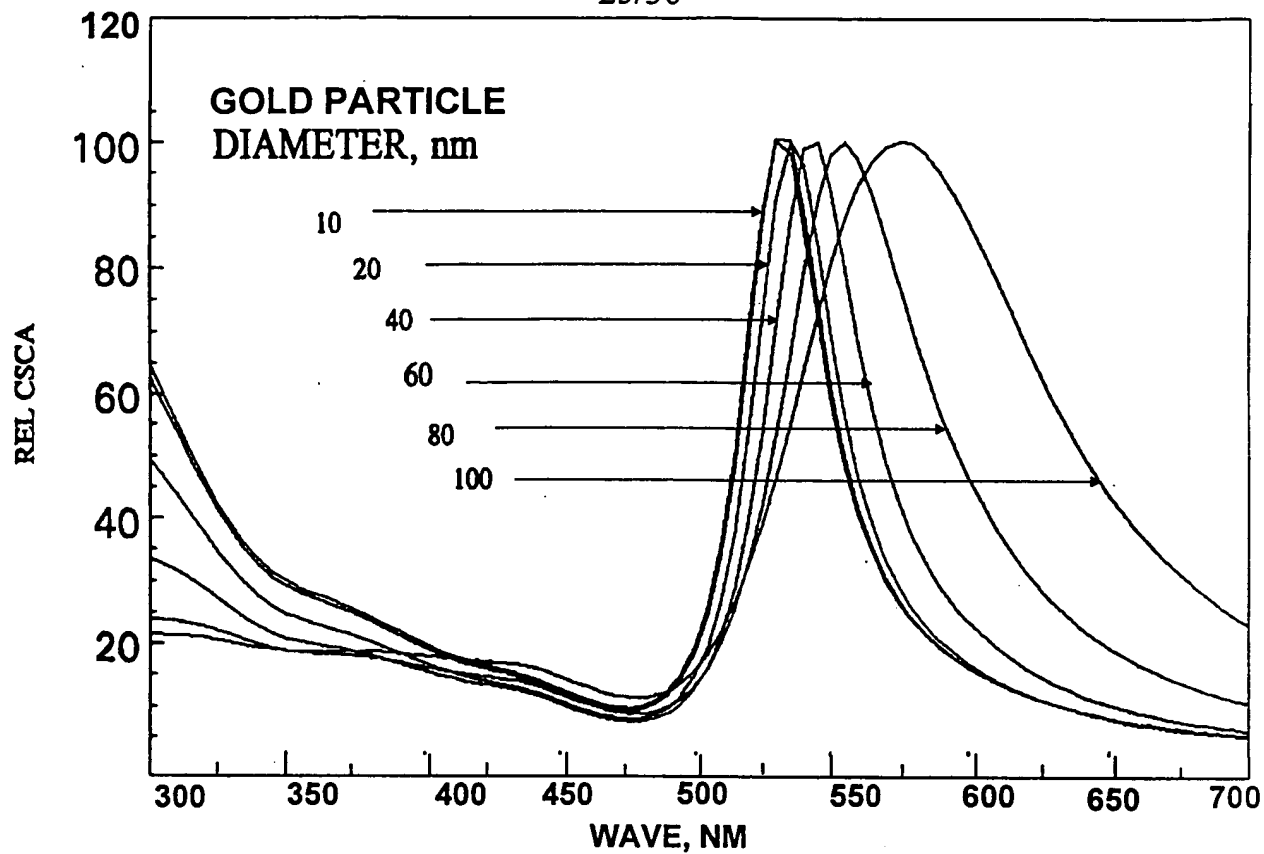


FIGURE 27

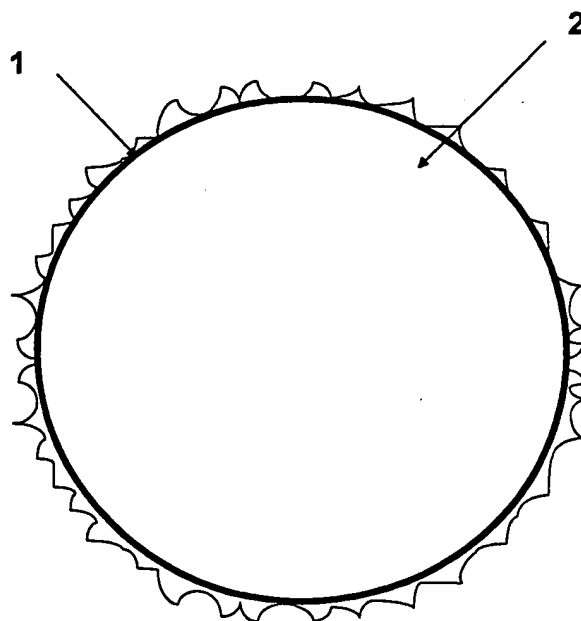


FIGURE 28

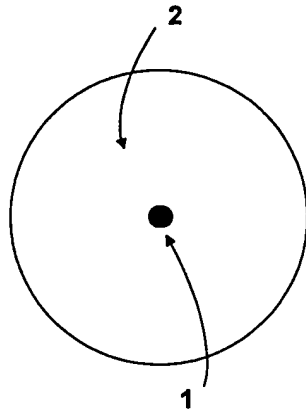


FIGURE 29A

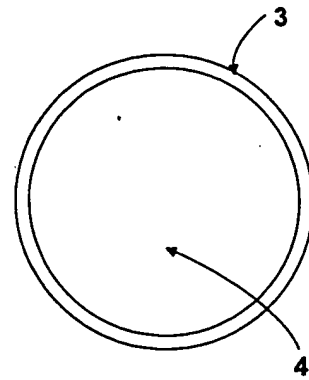


FIGURE 29B

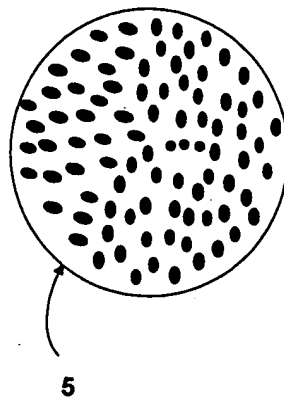


FIGURE 29C

00044729-004604

27/30

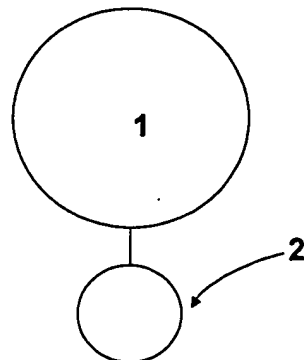


FIGURE 30A

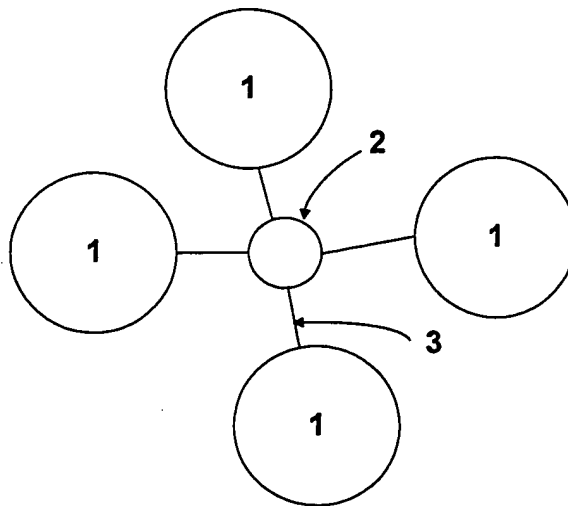


FIGURE 30B

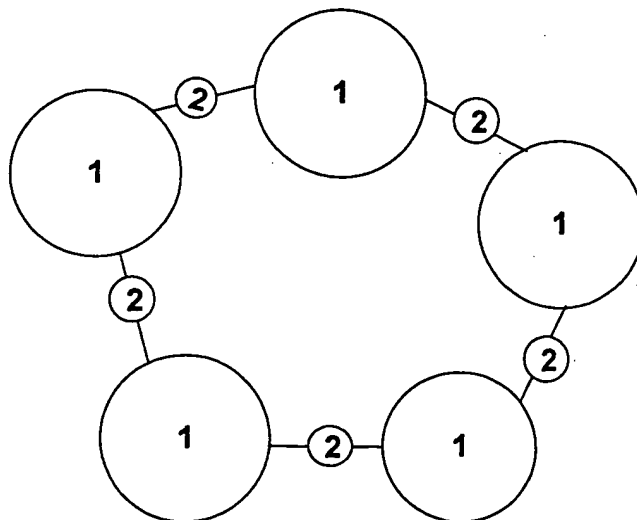


FIGURE 30C

409480-022 FEB 60

28/30

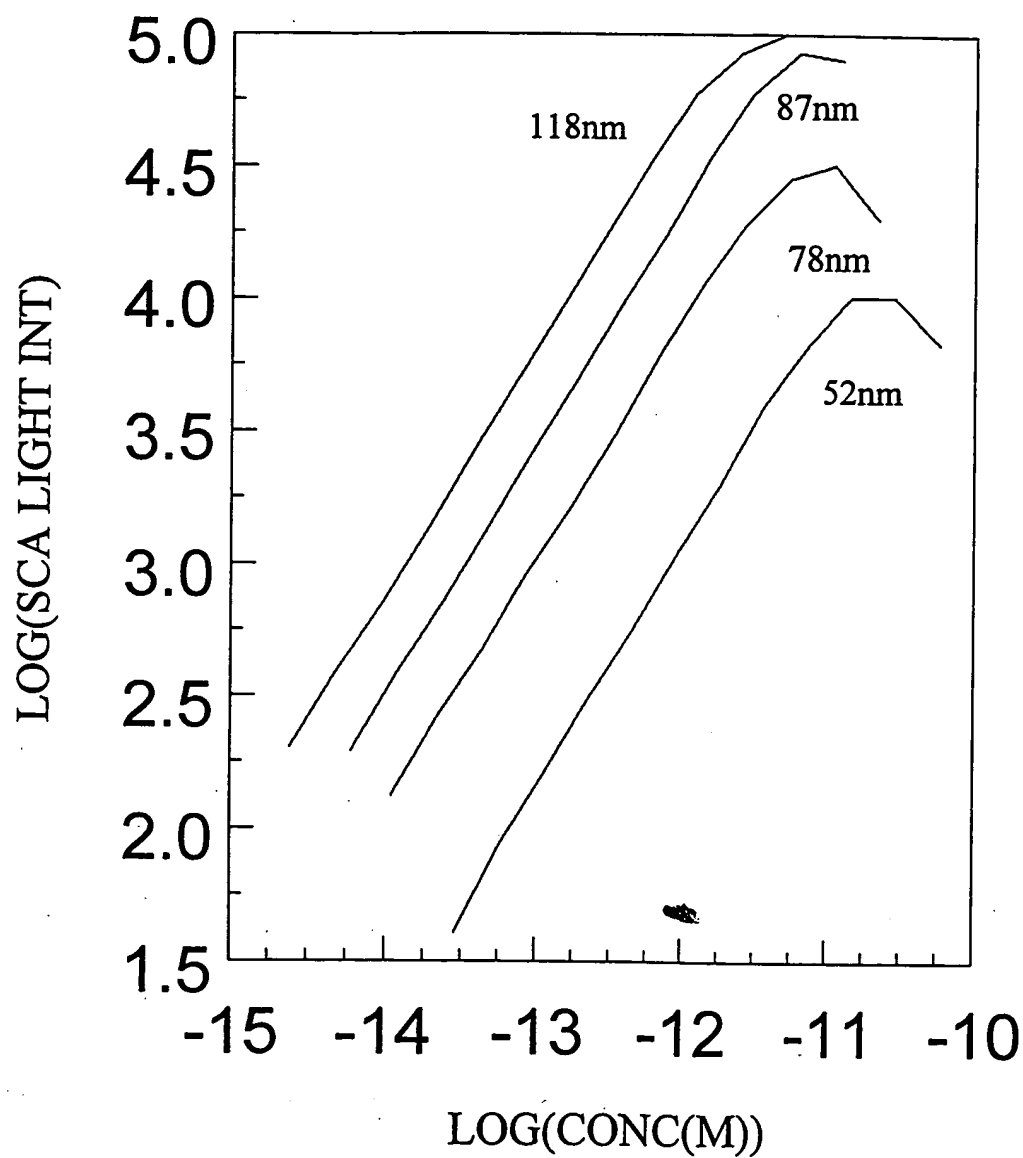


FIGURE 31

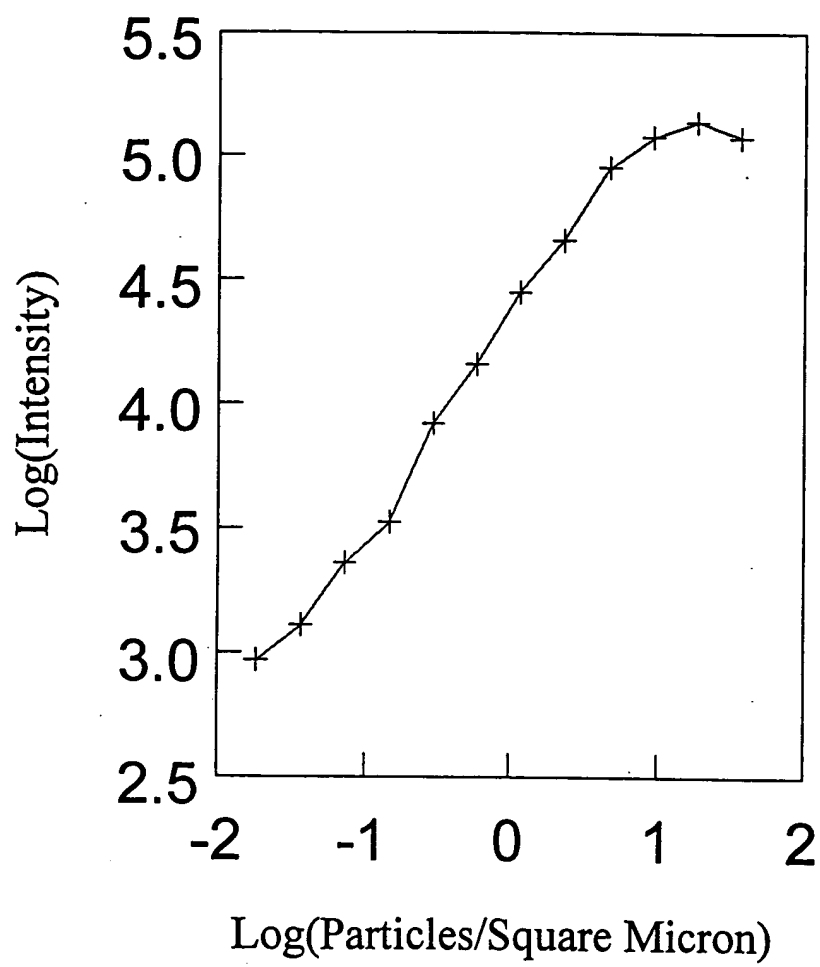


FIGURE 32

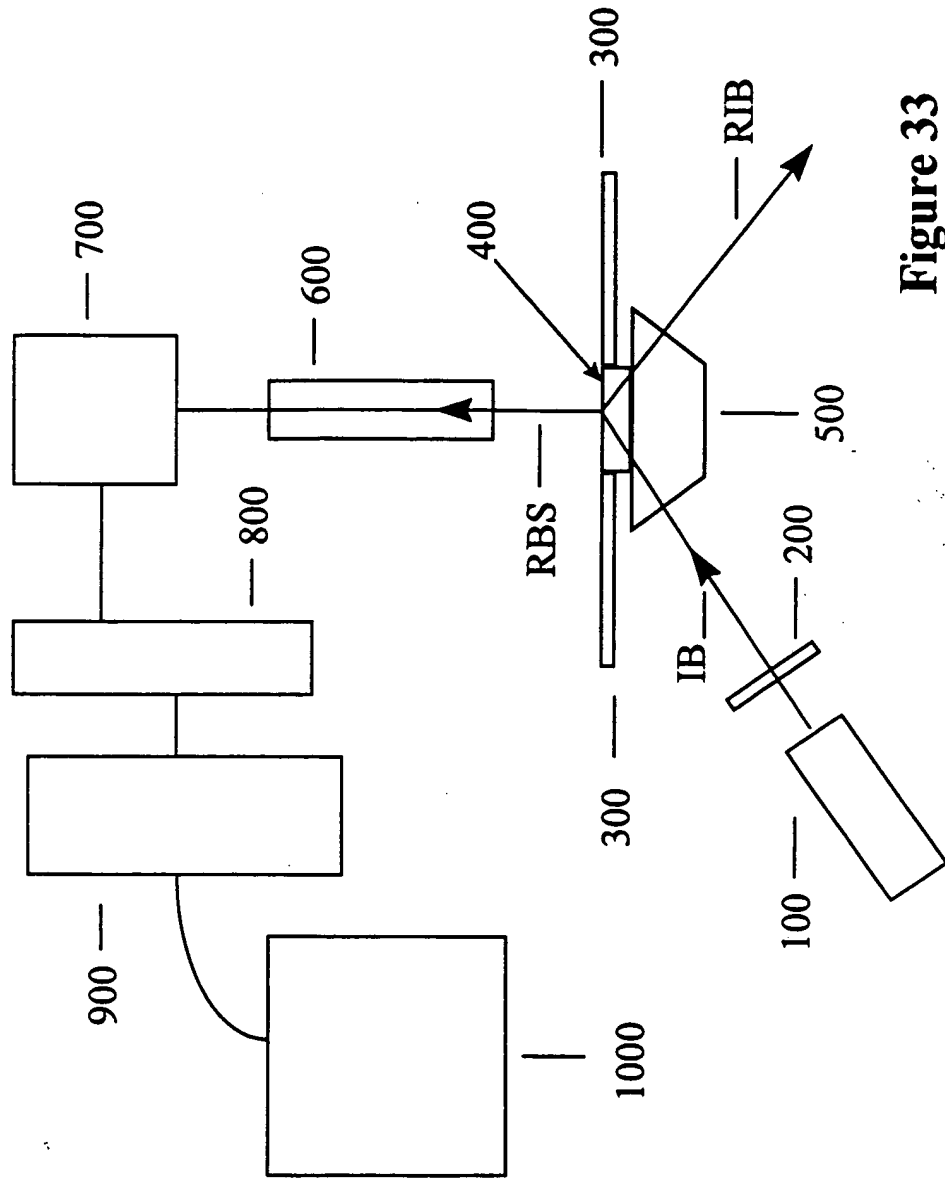


Figure 33